



MISSOURI DEPARTMENT OF HEALTH
STATE PUBLIC HEALTH LABORATORY
DATAMASTER MAINTENANCE REPORT

BREATH ALCOHOL PROGRAM **COPY**

JUN -9 2009

Complete this report in duplicate at the time of the regular monthly preventive maintenance check, and whenever instrument is repaired. Send copy to Department of Health; retain original in department file. **DNSS STATE HEALTH**

DATAMASTER SN **950124** DATE OF INSPECTION **06/06/09**

LOCATION OF INSTRUMENT (STREET AND CITY) **Kirksville Police Dept. 119 E. McPherson Kirksville, MO 63501-3505** TIME OF INSPECTION **10:26**

CHECKLIST: Place a check (✓) to the left of each item if found to be satisfactory or if operating within established limits. (Write in observed values where determined.) Unchecked items must be corrected before using instrument.

☒ **DIAGNOSTIC CHECK (PRINTOUT ATTACHED)**

☒ **COMPUTER**

☒ **DETECTOR**

☒ **PROGRAM**

☒ **FILTERS**

☒ **HEATERS SAMPLE CHAMBER** **49** °C

☒ **QUARTZ STANDARD**

☒ **FLOW DETECTOR**

☒ **CALIBRATION**

☒ **PUMP HIGH SPEED**

☒ **PRINTER**

☒ **INDICATOR LIGHTS**

☒ **TIME AND DATE**

Jun 06

10:28

☒ **SIMULATOR TEMPERATURE (34 °C ± 0.2°C)**

34.0° C

☒ **CALIBRATION CHECK -**

Run three tests using a standard solution. All three tests must be within ± 5% of the standard value and must have a spread of .005 or less. Check the box corresponding to the standard solution being used. (PRINTOUT ATTACHED) (USE RECIRCULATION PUMP)

☒ **0.100% STANDARD - MUST READ BETWEEN 0.095% and 0.105% INCLUSIVE**

☐ **0.040% STANDARD - MUST READ BETWEEN 0.038% and 0.042% INCLUSIVE**

(ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)

TEST 1 **.101**

TEST 2 **.101**

TEST 3 **.102**

☒ **PERFORM R.F.I. TEST (PRINTOUT ATTACHED)**

☒ **NUMBER OF REFUSALS, SINCE LAST MAINTENANCE REPORT, AND NUMBER OF BREATH TESTS IN EACH RANGE AS FOLLOWS: (DO NOT INCLUDE SIMULATOR TESTS)**

REFUSALS **0** (0-.04) **3** (.05-.09) **0** (.10-.14) **2** (.15-.19) **1** (Over .19) **1**

List any new parts and describe any alteration or modification that was made to restore the instrument to operate satisfactorily and within established limits (use other side if necessary)

INSTRUMENT OPERATES WITHIN D.H.S.S. SPECIFICATIONS

Simulator solution supplied by Repco. Lot #: 08002 Bottle #: 0628 Expiration date: 10/13/10

INSPECTING OFFICER

SIGNATURE

PRINT NAME

James Holzmeier

TYPE II PERMIT NUMBER/EXPIRATION DATE

820314

exp. 11/07/10

TELEPHONE NUMBER

660-785-6945 ext. 15

CERTIFICATE OF ANALYSIS

MANUFACTURER AND SUPPLIER: RepCo Marketing, Inc.

LOT NUMBER: 08002

EXPIRATION DATE: October 13, 2010 at 11:59 p.m.

RepCo Marketing, Inc. certifies the following:

RepCo Marketing, Inc. manufactured, tested and supplied Lot Number 08002 of Alcohol Certified Solution for simulators. Random samples of said lot number were analyzed utilizing a gas chromatograph and found to contain 0.1209 gms/dl wt/vol ethyl alcohol in aqueous solution (i.e. ethanol).

The alcohol and distilled water used in the solution were found to be free of any interfering substance.

This solution will produce a vapor alcohol value of 0.100% +/-3% when heated to 34 Degrees Celsius +/-0.2 Degrees Celsius in a simulator.

The date of manufacture for this lot number is October 14, 2008. The expiration date for this lot number is October 13, 2010 at 11:59 p.m.

This document is a true representation of the original Certificate of Analysis.



Cecil B. Garner, President
RepCo Marking, Inc.

Face This Side Down - This Edge In First

BAC DataMaster Evidence Ticket

KIRKSVILLE POLICE DEPARTMENT

BAC DATAMASTER SERIAL NUMBER 958124
06/06/09

TESTING OFFICER:
HOLZMEIER/JAMES
OFFICER I.D.: 123
PERMIT NUMBER: SP8314
EXPIRATION DATE: 11/37/10
MISCELLANEOUS DATA:

--- SUPERVISOR MODE ---

BLANK TEST	.000	10
INTERNAL STANDARD	VERIFIED	10
EXTERNAL STANDARD	.101	10
BLANK TEST	.000	10
EXTERNAL STANDARD	.101	10
BLANK TEST	.000	10
EXTERNAL STANDARD	.101	10
BLANK TEST	.000	10

N = 3
S.D. = .1
AVG. = .1013

Operator Signature

Face This Side Down - This Edge In First

BAC DataMaster Evidence Ticket

KIRKSVILLE POLICE DEPARTMENT

BAC DATAMASTER SERIAL NUMBER 958124
06/06/09
10:06

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
HEATERS	
SAMPLE CHAMBER:	49c
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

! " # \$ % ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~

Operator Signature

Face This Side Down - This Edge In First

BAC DataMaster Evidence Ticket

KIRKSVILLE POLICE DEPARTMENT

BAC DATA MASTER SERIAL NUMBER 959124
06/06/09

ARREST TIME: 09:00

SUBJECT NAME:

RFI/TEST

DOB: 01/01/01 SEX: M

STATE/D.L.: MO/N/A

ARRESTING OFFICER:

N/A

OFFICER I.D.: N/A

TESTING OFFICER:

HOLZMEIER/JAMES

OFFICER I.D.: 123

PERMIT NUMBER: 828314

EXPIRATION DATE: 11/07/10

MISCELLANEOUS DATA:


--- BREATH ANALYSIS ---

BLANK TEST .000 10:05

INTERNAL STANDARD VERIFIED 10:06

RADIO INTERFERENCE


Operator Signature

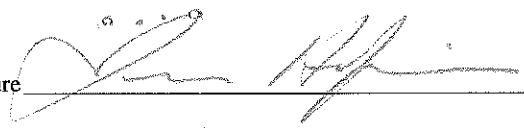

State of Missouri
DEPARTMENT OF HEALTH

COPY

PERMIT
TYPE II



JAMES L. HOLZMEIER

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field repairs, and operate the following breath analyzer(s):
INTOXILYZER 5000; DATAMASTER

for the determination of the alcoholic content of blood from a sample of expired (alveolar) air. Issued under the provisions of sections 577.020 through 577.041, RSMo 1986.

11/07/08

Date

820314

Number

11/07/2010

Expires

John J. Mathewson

Director of State Public Health Laboratory

Director, Department of Health

MO 580-0771 (7-88)

Lab. 4 (R7-88)